

---

---

**Urine-absorbing aids for  
incontinence — Polyacrylate  
superabsorbent powders —**

**Part 5:  
Test method for determination of  
the free swell capacity in saline by  
gravimetric measurement**

*Aides pour absorption d'urine — Méthodes d'essai pour caractériser  
les matériaux absorbants à base de polymères —*

*Partie 5: Détermination gravimétrique de la capacité de gonflement  
en solution saline*



STANDARDSISO.COM : Click to view the full PDF of ISO 17190-5:2020



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2020

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
Foreword .....	iv
1 Scope .....	1
2 Normative references .....	1
3 Terms and definitions .....	1
4 Principle .....	2
5 Reagents and materials .....	2
6 Apparatus .....	3
7 Conditioning .....	3
8 Sampling .....	3
9 Procedure .....	4
10 Calculation .....	5
11 Report .....	5
12 Precision .....	6
Bibliography .....	7

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 173, *Assistive products*, Subcommittee SC 3, *Aids for ostomy and incontinence*.

This second edition cancels and replaces the first edition (ISO 17190-5:2001), which has been technically revised. The main changes compared to the previous edition are as follows:

- full text review and new laboratory analysis with statistical evaluation;
- sample weighing simplified;
- request for duplication removed.

A list of all parts in the ISO 17190 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

# Urine-absorbing aids for incontinence — Polyacrylate superabsorbent powders —

## Part 5:

## Test method for determination of the free swell capacity in saline by gravimetric measurement

**WARNING** — This document does not claim to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this document to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use. It is expected that the person performing this test has been fully trained in all aspects of this procedure.

### 1 Scope

This document provides a test method that determines the free swell capacity of polyacrylate superabsorbent powders in saline solution.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 187, *Paper, board and pulps — Standard atmosphere for conditioning and testing and procedure for monitoring the atmosphere and conditioning of samples*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

### 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

#### 3.1

##### **sample**

product or portion of a product taken from a production lot for testing purposes and identifiable and traceable back to its origin

#### 3.2

##### **specimen**

specific portion of the identified *sample* (3.1) upon which a test is performed

## 4 Principle

The sample is weighed and placed in a water-permeable bag. The bag is submerged in the fluid to be absorbed and allowed to soak for a defined soaking period, after which the bag is removed. Excess fluid is allowed to drip away and the sample is weighed to determine the amount of fluid absorbed.

## 5 Reagents and materials

Use only reagents of recognized analytical grade, unless otherwise specified.

### 5.1 Water.

Grade 3 water in accordance with ISO 3696, with the exception that the conductivity can be as high as 30  $\mu\text{S}/\text{cm}$ .

### 5.2 Sodium chloride solution.

**5.2.1** 0,9 % mass fraction of sodium chloride solution in water. Weigh  $(9,00 \pm 0,01)$  g of sodium chloride into a 1 l beaker and add  $(991,0 \pm 0,1)$  g of deionized water (grade 3). Stir until dissolved.

**5.2.2** The conductivity of the solution should be checked prior to each use using properly calibrated measuring equipment. The expected conductivity of a 0,9 % saline solution is of the order of 1600 S/m at 25 °C. Each testing lab shall determine the correct conductivity for the conditions obtaining in the lab. It is also recommended that the temperature of the solution be maintained at  $(23 \pm 2)$  °C for the duration of the test. As this matches the required laboratory temperature, it is not necessary to record the solution temperature.

### 5.3 Nonwoven bag.

**NOTE** Bags described in this document are often referred to as “teabags”.

The bag has the external dimensions of  $(60 \times 40)$  mm<sup>2</sup> to  $(60 \times 85)$  mm<sup>2</sup> and is made of non-apertured heat-sealable nonwoven. One example of a suitable specification for the nonwoven is the following:

- Mass per unit area:  $(16,5 \pm 1,5)$  g/m<sup>2</sup>;
- Thermoplastic fibre content:  $(4,0 \pm 0,8)$  g/m<sup>2</sup>;
- Web tensile strength in cross direction:  $(70 \pm 12)$  N/m;
- Air permeability (4 plies tested):  $2,30 \pm 0,50$  l.min<sup>-1</sup>.cm<sup>-2</sup> at a pressure drop of 124 Pa.

Normally the teabag paper is supplied as a roll, for example 120 mm wide. This shall be stored flat as storing in an upright position (as a wheel) will compress the paper at bottom of the roll and affect its characteristics.

The teabag is made by cutting sections, for example 60 mm wide, which will provide teabags  $60 \times 60$  mm<sup>2</sup> when folded and sealed. In this example, the paper may be folded in half and sealed along two sides ready for the addition of superabsorbent powder and the sealing of the final side prior to running the test.

It is recommended to have teabags made in bulk and delivered ready-made for use in the lab.

In any case, teabags should be stored in cool, dry conditions. For best practice, storing teabags in a desiccator prior to use is also recommended.

## 6 Apparatus

**6.1 Bag**, having dimensions of  $(60 \times 40) \text{ mm}^2$  to  $(60 \times 85) \text{ mm}^2$  and made of non-apertured heat-sealable nonwoven. Fold the nonwoven and heat-seal two of three open sides about 3 mm to 5 mm from the open edges to obtain the bag. Each experimental set comprises two bags per test sample.

**6.2 Heat sealer**, capable of bonding nonwoven.

**6.3 Large pan with cover**,  $>5 \text{ cm}$  internal depth and large enough to hold several bags. A compartmentalized tray is recommended to keep each teabag separate from the others, but the compartments shall be large enough to allow the teabag to be properly submerged and where swelling is not restricted by the volume of the compartment.

**6.4 Analytical balance**, capable of weighing a mass of between  $(0,80 \pm 0,001) \text{ g}$  and  $(0,220 \pm 0,001) \text{ g}$  of polymer powder in combination with the mass of the teabag (if weighed directly) or weighing vessel or laboratory paper employed.

**6.5 Analytical balance**, capable of weighing a mass of  $(9,00 \pm 0,01) \text{ g}$  of sodium chloride in combination with the mass of the weighing vessel or laboratory paper employed.

**6.6 Analytical balance**, capable of weighing a mass of  $(1\,000,00 \pm 1,00) \text{ g}$  of sodium chloride solution in combination with the mass of the vessel employed.

**6.7 Weighing vessel or laboratory paper**.

**6.8 Metal spatula**, to accommodate  $0,2 \text{ g}$  of superabsorbent powder.

**6.9 Timer**, accurate to 1 second in 30 minutes.

**6.10 Drying rack or line with clips**.

**6.11 Volumetric flask**, of  $1 \text{ l}$  capacity and Grade "A" quality.


## 7 Conditioning

Samples shall be delivered in a closed container, to prevent absorption of atmospheric moisture. Allow the closed container to equilibrate to the laboratory conditions. The preferred test conditions are  $(23 \pm 2) ^\circ\text{C}$  and  $(45 \pm 15) \%$  relative humidity. If these conditions are not available, test at ambient conditions and report the temperature and relative humidity. Measure these laboratory conditions in accordance with ISO 187.

## 8 Sampling

**WARNING — Powder Handling** – The German Commission for the Investigation of Health Hazards of Chemical Compounds in the Work Area (MAK Commission) has provided a guideline value for long-term exposure to the respirable portion of superabsorbent polyacrylate dust of  $0,05 \text{ mg.m}^{-3}$ . The respirable portion is defined as those particles of less than  $10 \mu\text{m}$  diameter. Commercial superabsorbent polymers typically contain less than  $0,1 \%$  of such particles. Precautions should be taken to avoid routine exposure to atmospheric respirable particles above this guideline value.

**8.1** Before taking a test portion out of the container to run the test, rotate the container five to ten times in a three-dimensional figure of eight motion (see [Figure 1](#)), so as to obtain a homogeneous product. For that matter, sample bottles should not be filled more than 80 % of their nominal capacity.

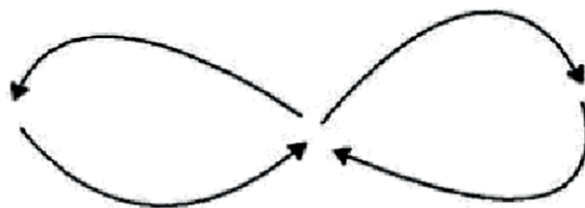

**Figure 1 — Sense of motion of the container**

**8.2** Make sure the test portion is substantially free of lumps of size greater than 1 mm in diameter before proceeding with testing. Lumps can pierce the screen and disqualify the equipment and the test.

## 9 Procedure

**9.1** If necessary, prepare the teabags.

**9.2** Place a teabag onto the balance pan and tare the balance.

**9.3** Add between 0,180 and 0,220 g of superabsorbent test sample into the teabag.

Transfer the sample portion from the sample bottle to the weighing vessel or laboratory paper in one spatula portion. Discard any excess material on the spatula. Do not return it to the sample bottle. Keep the sample container closed as much as possible during this process.

**9.4** Record the weight of the dry polymer as  $ms_1$ .

**9.5** Seal the teabag (the seam should be about 5 mm from open side of the teabag).

**9.6** Use the same procedure to prepare a second test portion and record the mass as  $ms_2$ .

**9.7** If it takes longer than 5 minutes to weigh and seal the bags before starting the test, place the bags in a desiccator.

**9.8** Prepare 2 blank bags and test alongside the bags containing polymer.

**NOTE** As long as bag materials and sealing conditions are unchanged, the use of historical data on the blanks can be considered. In this case, the tests on the two blanks need not be carried out. However, regular (daily) checking of the blank teabags is advised for quality control checking.

**9.9** Fill the pan with 0,9 % saline solution, using at least 1 litre of saline per 10 teabags.

Use fresh saline for each batch of teabags tested as the saline can become more concentrated owing to water evaporation during the test and contaminated by water soluble extractables from the polymer samples. Otherwise gives wrong answer.

**9.10** Hold each bag containing the test portion by its opposite edges and evenly distribute the test portion horizontally throughout the bag.

**9.11** Lay each bag on the surface of the saline solution.



**9.12** After each tea bag has become fully wet for (typically about one minute), gently push it under the liquid surface.

**9.13** Eliminate any entrapped air bubbles by manipulating the bag.

**9.14** Allow the test portion to absorb the saline solution for a period of 30 minutes.

**9.15** At the end of the immersion period, remove each bag from the tray of saline solution and hang diagonally on a line from one of the double-sealed corners for 10 minutes, so as to remove excess saline solution by dripping.

**9.16** Discard the saline solution.

**9.17** Weigh each bag and record the mass of the two blank bags  $m_{b1}$  and  $m_{b2}$ , and the mass of the bags containing polyacrylate superabsorbent gel  $m_{w1}$  and  $m_{w2}$ .

## 10 Calculation

Calculate the average of the two blank values:

$$m_b = \frac{(m_{b1} + m_{b2})}{2}$$

For each sample, ( $i = 1$  or  $2$ ), calculate the free swell capacity,  $w_i$ , expressed as a mass fraction (g/g):

$$w_i = \frac{(m_{wi} - m_b) - m_{si}}{m_{si}}$$

where

$m_{si}$  is the mass, expressed in grams, of dry test portion

$m_b$  is the average mass, expressed in grams, of the 2 wet blank bags

$m_{wi}$  is the mass, expressed in grams, of the wet bag containing polyacrylate superabsorbent powder

## 11 Report

In addition to the precise test results, the report shall include the following information:

- a) Reference to this document, i.e. ISO 17190-5:2020;
- b) Complete identification of all materials tested and method of sampling;
- c) Name and address of testing institution;
- d) Make and model of testing equipment;
- e) The type of polymer-based absorbent materials, including all technical details and source information required for complete identification of the sample;
- f) The results of the free swell capacity in saline solution for each test portion, expressed as mass fraction in grams per gram (g/g) to the nearest 0,1 g/g and the average for duplicate determinations;
- g) Laboratory testing conditions;
- h) Number of specimens tested;